Chromatogram and Results

Injection Details

Injection Name:	**YT307-I2**	*Run Time (min):*	**10.17**
Vial Number:	**GA5**	*Injection Volume:*	**1.00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**254**
Instrument Method:	**YT307**	*Bandwidth:*	**4**
Processing Method:	**3D Quantitative**	*Dilution Factor:*	**1.0000**
Injection Date/Time:	**2023/2/10 15:48:07 ÉÏÏç**	*Sample Weight:*	**1.0000**

Chromatogram

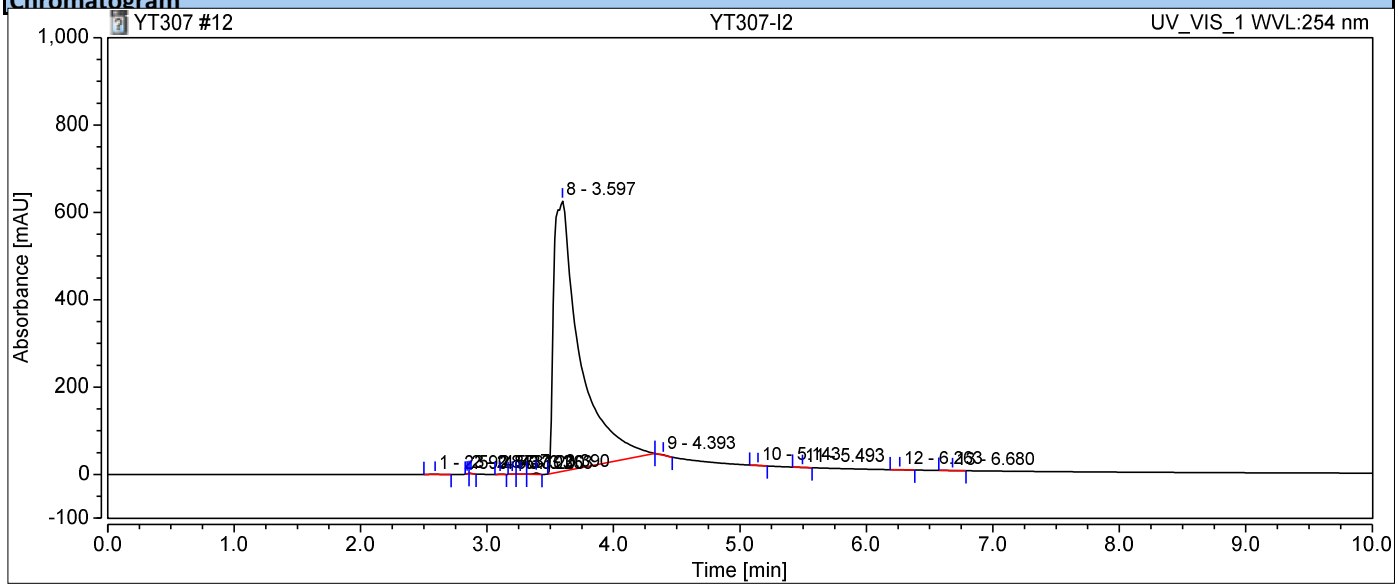

MS Results

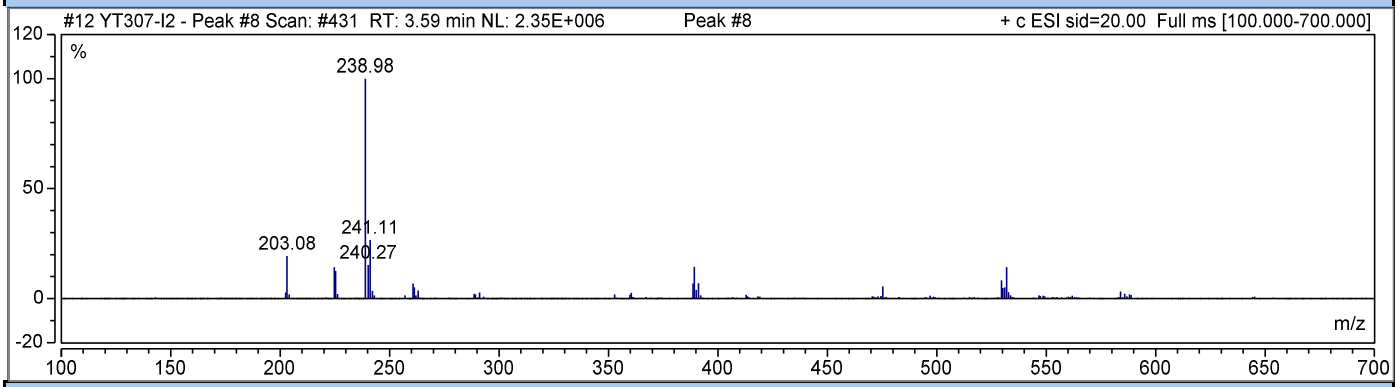

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount n.a.
1		2.590	0.037	0.425	0.0245	0.07	n.a.
2		2.843	0.003	0.202	0.0022	0.03	n.a.
3		2.873	0.022	0.811	0.0147	0.13	n.a.
4		3.103	0.015	0.340	0.0103	0.05	n.a.
5		3.200	0.006	0.166	0.0037	0.03	n.a.
6		3.263	0.009	0.191	0.0062	0.03	n.a.
7		3.390	0.153	3.727	0.1028	0.59	n.a.
8		3.597	148.906	619.350	99.7735	98.84	n.a.
9		4.393	0.059	0.921	0.0396	0.15	n.a.
10		5.143	0.016	0.253	0.0108	0.04	n.a.
11		5.493	0.007	0.088	0.0045	0.01	n.a.
12		6.263	0.005	0.068	0.0035	0.01	n.a.

13		6.680	0.005	0.059	0.0037	0.01	n.a.
Total:			**149.244**	**626.601**	**100.00**	**100.00**	